



Test Report/ Certificate of Analysis


Date of Report Mar 27, 2026

To: MHS Longevity

From: AxisPharm, LLC

Certificate ID Number: 27Mar2026-03

Results reported by: Lab Technician
Ning Yang

Review/Approved by: 
QA Director
Dawei Yue

Sample Received: Date: 03/23/2026
Receiving Condition: Acceptable Other: _____
Storage Condition: Room temperature -20°C -80°C
 Other: __ 0 °C _____


Method(s): LCMS, LAL Endotoxin Assay, and ICP-MS for trace heavy metal

Procedure(s): Laboratory Activity Date: 3/23/2026-03/27/2026

Results:



Test Report/ Certificate of Analysis

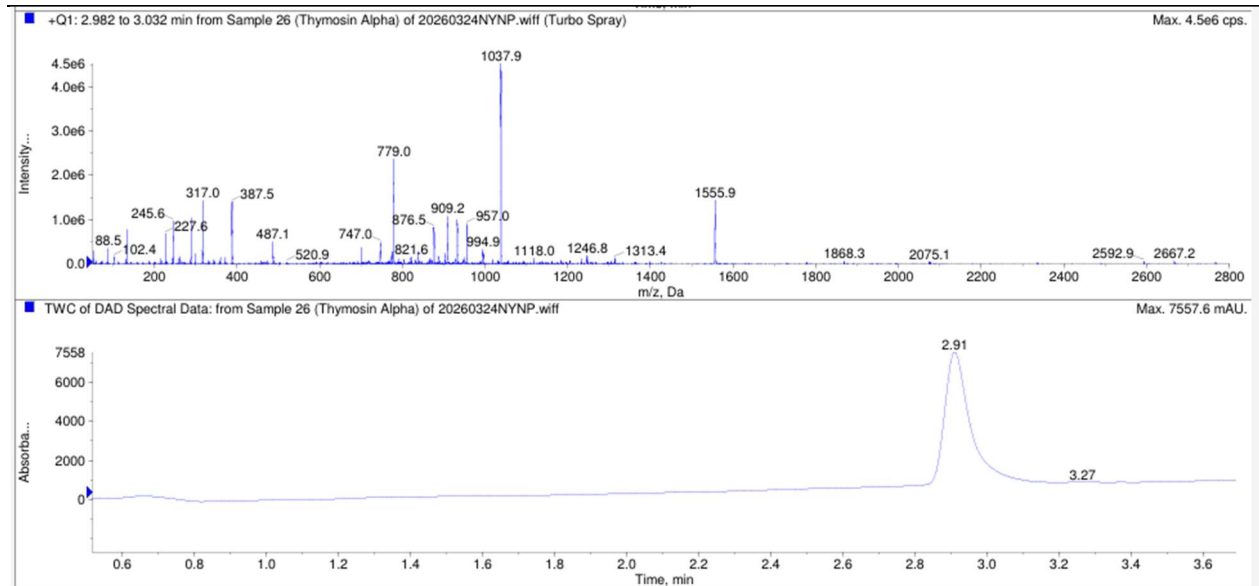

Sample Name	Net Weight Measured	MW (g/mol)	Detected	UV Purity (220nm) (%)
DSIP 10mg	10.1mg	848.8	850.3[M+H]	>99.5

Endotoxin Results:

Sample Name	Endotoxin Testing Value (EU/mg)
DSIP 10mg	0.057

ICP-MS

Element	Sym.	DL (ppm)	ppm
Antimony	Sb	0.15	<0.15
Arsenic	As	0.15	<0.15
Cadmium	Cad	0.15	<0.15
Cobalt	Co	0.15	<0.15
Copper	Cu	0.15	<0.15
Lead	Pb	0.15	<0.15
Mercury	Mg	0.15	<0.15
Nickel	Ni	0.15	<0.15
Vanadium	V	0.15	<0.15

Preservatives, salts and sugars that serves as fillers in injectables are not considered as impurities. Conclusion: The product comes with DSIP 10.1mg with purity >99.5%.